

ATTX110



FIXED PROBE THERMOMETER

Product Code: ATTX110


Klipspringer

Compliance with confidence

t/ +44 (0)1473 461 800
e/ service@klipspringer.com

www.klipspringer.com

Klipspringer Ltd
Rynor House, Farthing Road, IPSWICH, UK, IP1 5AP

This page is intentionally left blank.

TABLE OF CONTENTS

1.	INTRODUCTION	4
2.	CAUTION	4
3.	OPERATION	4
4.	TEMPERATURE MEASUREMENT	5
5.	BATTERIES	5
6.	STORAGE AND CLEANING	6
7.	ERROR MESSAGES	6
8.	SPECIFICATIONS	6
9.	DISPOSAL	7
10.	WARRANTY STATEMENT	7

1.0 INTRODUCTION

- 1.1 Congratulations on your purchase of this fixed probe thermometer. We hope that you can make use of this product for a long time and it helps you with your work.
- 1.2 Powered by a replaceable lithium battery, the thermometer is a handy, temperature measurement device for a whole range of measurement and control applications.

2.0 CAUTION

The thermometer must be protected from the following:

- 2.1 Electrostatic discharge
- 2.2 Thermal shock caused through sudden extreme ambient temperature changes. Allow instrument to stabilise for up to 30 seconds when

affected or when moving into extreme changes in ambient temperatures.

2.3 Do not leave the unit on or near objects of high temperature.

2.4 Keep out of reach of all children.

3.0 OPERATION

(1) LCD Display


(2) ON/HOLD

(3) °C/°F switch



3.1 To switch ON press and keep the ON/HOLD (2) for approximately one second.

3.2 LCD display (1); all the necessary information is displayed on the LCD. The individual symbols have the following meanings:




(1) Current Temperature measurement

(2) Minus symbol for negative measurement values

(3) Battery status indicator

(4) "HOLD" (Auto shut down after 10 minutes)

(5) Unit of measurement (°C/°F)



3.3 Select the required unit of measurement °C or °F.

- Switch on the device by pressing ON/HOLD (2). As soon as 'Ebro' is shown, press ON/HOLD (2) again for 3 seconds and release. The settings menu is active, and the current unit is shown.
- Press ON/HOLD (2) once, the display will switch to the next unit.
- Press ON/HOLD (2) for more than 2 seconds, the current unit will be stored, and then the settings menu will be left.

4.0 TEMPERATURE MEASUREMENT

4.1 As soon as you switch on the device, it starts to take a temperature reading every second.

- 4.2 Press ON/HOLD (2) once, the device stops measuring and the last reading is shown on the LCD display. (“HOLD” is shown on the LCD)
- 4.3 Press ON/HOLD (2) again, the device starts measuring again.

*The last measured value is frozen, and the thermometer deactivates itself automatically after about 10 minutes to save battery power.


5.0 BATTERIES

5.1 The thermometer incorporates visual low battery indication as follows:



5.2 Battery replacement: when the ‘Low battery’ icon indicates the battery is low, the battery should be replaced immediately.

5.3 Remove battery cover (1) from the back of the thermometer using a coin or equivalent. Insert new CR2032 battery and replace cover.

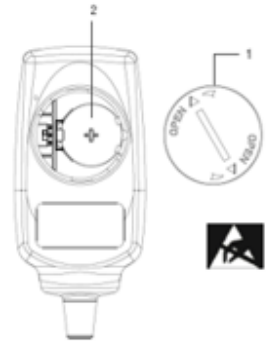

Please note: it is important to turn the instrument off before replacing the battery otherwise the thermometer may malfunction.

6.0 STORAGE AND CLEANING

- 6.1 Clean the device with a damp cloth. Do not use any solvents such as Acetone as they corrode the plastic. Isopropyl alcohol may be used to disinfect.
- 6.2 Do not submerge any part of the thermometer.
- 6.3 The thermometer should be stored at room temperature between -20 to +65°C (-4 to 149°F).

7.0 ERROR MESSAGES

“Hi” Temperature measured is above +350°C/+1200°C



“Lo” Temperature measured is below -50°C/-60°F

“Er2” Too quick a change in ambient temperature



“Er3” Ambient temperature below -20°C or above +50°C.
Bring thermometer within operating temperature range
and allow 30 minutes to stabilise.



“Er” All other errors.

Reset the thermometer by removing the battery for 2 minutes.

8.0 SPECIFICATIONS

Accuracy	± 0.8°C or ± 0.8 % whichever is greater
IP rating	IP55
Probe dimensions	90mm x 3.0mm
Sensor	Thermocouple Type T
Warranty	2 years
Dimensions (mm)	182 x 42 x 17mm
Resolution	0.1°C
Measuring range	-50...+350°C
Storage temperature	-30 °C...+70 °C
Probe type	Penetration
Battery	3v CR2032
Certification	Free issue certificate supplied

9.0 DISPOSAL

9.1 Instrument is subject to WEEE directive and must be disposed off appropriately. For further information or advice contact Klipspringer.

11.0 WARRENTY STATEMENT

- 11.1. This product has a 2-year manufacturer's warranty against defective manufacturing, with the exception of the battery.

